

Optical coherence tomography of cell dynamics in three-dimensional tissue models

Wei Tan, Amy L. Oldenburg

*Biophotonics Imaging Laboratory
Beckman Institute for Advanced Science and Technology
Department of Electrical and Computer Engineering
University of Illinois at Urbana-Champaign*

Stephen A. Boppart

*Biophotonics Imaging Laboratory
Beckman Institute for Advanced Science and Technology
Department of Electrical and Computer Engineering,
Department of Bioengineering, Department of Internal Medicine
University of Illinois at Urbana-Champaign
405 N. Mathews Avenue, Urbana, IL 61801
boppart@uiuc.edu*

Abstract: Three-dimensional cell-based tissue models have been increasingly useful in the field of tissue engineering, drug discovery, and cell biology. While techniques for building these tissue models have been advanced, there have been increasing demands for imaging techniques that are capable of assessing complex dynamic three-dimensional cell behavior in real-time and at larger depths in highly-scattering scaffolds. Understanding these cell behaviors requires advanced imaging tools to progress from characterizing two-dimensional cell cultures to complex, highly-scattering, thick three-dimensional tissue constructs. Optical coherence tomography is an emerging biomedical imaging technique that can perform cellular-resolution imaging *in situ* and in real-time. In this study, we demonstrate that it is possible to use OCT to evaluate dynamic cell behavior and function in a quantitative fashion in four dimensions (three-dimensional space plus time). We investigated and characterized in thick tissue models a variety of cell processes, such as chemotaxis migration, proliferation, de-adhesion, and cell-material interactions. This optical imaging technique was developed and utilized in order to gain new insights into how chemical and/or mechanical microenvironments influence cellular dynamics in multiple dimensions. With deep imaging penetration and increased spatial and temporal resolution in three-dimensional space, OCT will be a useful tool for improving our understanding of complex biological interactions at the cellular level.

©2006 Optical Society of America

OCIS codes: (170.4500) Optical coherence tomography; (170.6900) Three-dimensional microscopy; (170.5380) Physiology; (170.1530) Cell analysis

References and links

1. R. Langer and J. P. Vacanti, "Tissue engineering," *Science* **260**, 920 (1993).
2. M. J. Friedrich, "Studying cancer in three dimensions," *JAMA* **290**, 1977 (2003).
3. D. J. Stephens and V. J. Allan, "Light microscopy techniques for live cell imaging," *Science* **300**, 82 (2003).
4. R. G. M. Breuls, A. Mol, R. Petterson, C. W. J. Oomens, F. P. T. Baaijens, and C. V. C. Bouten, "Monitoring local cell viability in engineered tissues: A fast, quantitative, and nondestructive approach," *Tissue Eng.* **9**, 269 (2003).

5. D. S. Gareau, P. R. Bargo, W. A. Horton, and S. L. Jacques, "Confocal fluorescence spectroscopy of subcutaneous cartilage expressing green fluorescent protein versus cutaneous collagen autofluorescence," *J. Biomed. Opt.* **9**, 254 (2004).
 6. B. R. Masters, P. T. So, and E. Gratton, "Multiphoton excitation microscopy of *in vivo* human skin. Functional and morphological optical biopsy based on three-dimensional imaging, lifetime measurements and fluorescence spectroscopy," *Ann. N. Y. Acad. Sci.* **838**, 58 (1998).
 7. P. T. So, C. Y. Dong, B. R. Masters, and K. M. Berland, "Two-photon excitation fluorescence microscopy," *Ann. Rev. Biomed. Eng.* **2**, 399 (2000).
 8. I. Constantinidis, C. L. Stabler, R. Long, and A. Sambanis, "Noninvasive monitoring of a retrievable bioartificial pancreas *in vivo*," *Ann. N. Y. Acad. Sci.* **961**, 298 (2002).
 9. A. S. P. Lin, T. H. Barrows, S. H. Cartmella, and R. E. Guldberg, "Microarchitectural and mechanical characterization of oriented porous polymer scaffolds," *Biomaterials* **24**, 481 (2003).
 10. D. Huang, E. A. Swanson, C. P. Lin, J. S. Schuman, W. G. Stinson, W. Chang, M. R. Hee, T. Flotte, K. Gregory, C. A. Puliafito, and J. G. Fujimoto, "Optical coherence tomography," *Science* **254**, 1178 (1991).
 11. B. E. Bouma and G. J. Tearney, editors, *Handbook of Optical Coherence Tomography*. Marcel Dekker, N.Y. (2001).
 12. J. M. Schmitt, "Optical coherence tomography (OCT): a review," *IEEE J. Select. Topics. Quantum Electron.* **5**, 1205 (1999).
 13. J. G. Fujimoto, "Optical coherence tomography for ultrahigh resolution *in vivo* imaging," *Nat. Biotechnol.* **21**, 1361 (2003).
 14. S. A. Boppart, B. E. Bouma, C. Pitris, J. F. Southern, M. E. Brezinski, and J. G. Fujimoto, "*In vivo* cellular optical coherence tomography imaging," *Nat. Med.* **4**, 861 (1998).
 15. A. G. Podoleanu, J. A. Rogers, D. A. Jackson, and S. Dunne, "Three dimensional OCT images from retina and skin," *Opt. Express* **7**, 292 (2000), <http://www.opticsinfobase.org/abstract.cfm?URI=oe-7-9-292>.
 16. S. A. Boppart, M. E. Brezinski, B. E. Bouma, G. J. Tearney, and J. G. Fujimoto, "Investigation of developing embryonic morphology using optical coherence tomography," *Dev. Biol.* **177**, 54 (1996).
 17. S. A. Boppart, G. J. Tearney, B. E. Bouma, J. F. Southern, M. E. Brezinski, and J. G. Fujimoto, "Noninvasive assessment of the developing *Xenopus* cardiovascular system using optical coherence tomography," *Proc. Natl. Acad. Sci. USA* **94**, 4256 (1997).
 18. X. Xu, R. K. Wang, and A. El Haj, "Investigation of changes in optical attenuation of bone and neuronal cells in organ culture or three-dimensional constructs *in vitro* with optical coherence tomography: relevance to cytochrome oxidase monitoring," *Eur. Biophys. J.* **32**, 355 (2003).
 19. C. Mason, J. F. Markusen, M. A. Town, P. Dunnill, and R. K. Wang, "The potential of optical coherence tomography in the engineering of living tissue," *Phys. Med. Biol.* **49**, 1097, 2004.
 20. H. Michna, "Induced locomotion of human and murine macrophages: a comparative analysis by means of the modified Boyden-chamber system and the agarose migration assay," *Cell Tissue Res.* **255**, 423 (1989).
 21. D. L. Marks, A. L. Oldenburg, J. J. Reynolds, S. A. Boppart, "Study of an ultrahigh-numerical-aperture fiber continuum generation source for optical coherence tomography," *Opt. Lett.* **27**, 2010 (2002).
 22. H. Steller, "Mechanisms and genes of cellular suicide," *Science* **267**, 1445 (1995).
 23. P. A. DiMilla, J. A. Quinn, S. M. Albelda, and D. A. Lauffenburger, "Measurement of individual cell migration parameters for human tissue cells," *Amer. Inst. Chem. Engr. J.* **38**, 1092 (1992).
 24. E. Cukierman, R. Pankov, D. R. Stevens, and K. M. Yamada, "Taking cell-matrix adhesions to the third dimension," *Science* **294**, 1708 (2001).
-

1. Introduction

Cell activities in three-dimensional (3-D) tissue models are of great interest for both basic cell biology research and applications, such as tissue engineering and pharmacological research [1,2]. Invasive imaging methods such as histology and scanning electron microscopy are used predominantly to evaluate cell activities and cellular responses to environmental stimuli in tissue models. These destructive methods, however, have intrinsic disadvantages. These methods do not permit real-time or dynamic imaging, lack real 3-D information, require long and harsh processing steps at discrete time points, and make structure–function correlations difficult. Consequently, despite tremendous increasing interest in this area, few have investigated the dynamics of cell behaviors in tissue models. The primary limitation has been inadequate imaging technology for high-resolution, real-time, noninvasive imaging deep within highly-scattering tissues.

Confocal microscopy has been an important advance in microscopy and has enabled the imaging of intact, optically nontransparent specimens to produce high-resolution (submicron) images of tissue structure with the use of fluorescent probes [3-5]. For a relatively thick specimen, confocal microscopy accomplishes optical sectioning by scanning the specimen with a focused beam of light and collecting the fluorescence signal via a pinhole aperture that spatially rejects light from out-of-focus areas of the specimen. Imaging depths, however, are limited to approximately one-hundred microns and exogenous fluorescence probes are usually required for detection, often limiting the long-term viability of the cells being imaged. Multiphoton microscopy, which relies on the simultaneous absorption of two or more near-infrared photons from a high-intensity short-pulse laser (most commonly a mode-locked titanium:sapphire laser) extends the imaging depth of confocal, but still with depth limitations of about 400–500 μm [6,7]. Newer technologies for imaging tissue models, including high-field-strength magnetic resonance imaging and microcomputed tomography, have been pursued for the assessment of cell and scaffold structure, with limited success. These techniques, with long data acquisition rates, hazards associated with high-energy radiation, and relatively high costs, are less suitable for both real-time and long-term imaging [8,9].

Optical coherence tomography (OCT) is an emerging technique that has the potential for overcoming many of the limitations of the current technologies [10,11]. OCT combines the high resolutions of most optical techniques with an ability to reject multiply-scattered photons and, hence, image at cellular resolutions (several microns) up to several millimeters deep in nontransparent (highly-scattering) tissue. Because OCT relies on variations in indices of refraction and optical scattering for image contrast, no exogenous fluorophores are necessary, enabling cellular imaging within living specimens over time without loss of viability. Because of longer wavelength, near-infrared light is scattered less than visible light, thus enhancing visualization of changes at greater depths. OCT has been applied *in vivo* for imaging the microstructures of different tissues including the eye, skin, gastrointestinal tracts, and neural systems, to name only a few, and is becoming a promising and powerful imaging technology that has widespread applications throughout many fields of medicine and biology [12-17]. However, few studies have investigated the use of the OCT technology for monitoring cell dynamics in tissue models for tissue engineering [18,19].

In this article, we report the use of OCT as a noninvasive imaging modality to explore 3-D cell activities in tissue models. OCT is capable of clearly identifying cells, and determining their position, distribution and general morphology in 3-D. For the first time, we investigate and characterize cell dynamics and processes including chemotaxis migration, proliferation, de-adhesion, and cell-material interactions. This optical imaging technique was developed and utilized in order to gain new insights into how chemical microenvironments influence cellular functions and dynamics in multi-dimensional models. Compared to other microscopy approaches, OCT permits high-resolution, real-time, deep-tissue, 3-D imaging to be performed rapidly and repeatedly over extended periods of time with intact, living tissue models, with the potential to extend imaging of scaffolds to *in vivo* applications, such as following grafting of engineered tissues into a host tissue.

2. Materials and Methods

2.1 Cell and Engineered Tissue Cultures

Tissue models are composed of cells, and matrix scaffolds or synthetic polymer scaffolds. In this study, NIH 3T3 cells (American Type Culture Collection [ATCC], Manassas, VA), green-fluorescent-protein (GFP)-vinculin transfected fibroblasts, and macrophages were used in our investigations. Gel-based tissue models were prepared by mixing cell suspension with thawed Matrigel solution (BD Bioscience, Bedford, MA) using 1:1 proportion, and then solidifying it in the 37 °C incubator. Other components such as collagen I (BD Bioscience, Bedford, MA) were added to the gel with appropriate weight proportions to study the effects

of matrix components on the OCT images. Cell and tissue cultures were maintained in an incubator at 37 °C and with 5% CO₂. For real-time imaging over extended time periods (days), tissue cultures were maintained in a portable microincubator (LU-CPC, Harvard Apparatus, Holliston, MA) that was placed on the microscope stages.

2.2 Cell Migration Assay

Matrigel-based invasion assays are a representative method of *in vivo* events. Porous filters were coated with 3 mm-thick Matrigel layer and placed in a custom-made two-chamber system, modified from the Boyden migration chamber design [20]. Macrophage chemo-attractant, 100 nM of monocyte chemo-attractant protein-1 (MCP-1, Research Diagnostics Inc, NJ), was placed in the lower chamber and macrophages and Matrigel were placed in the upper chamber. Before beginning the migration assay, macrophages were starved in serum-free media for ~12 hrs. Then, the cell suspension containing 1×10^5 cells was mixed with Matrigel gel to form a layer in the top chamber. The migration chamber was incubated in a humidified 5% CO₂, 37 °C incubator for 2-3 hrs, before transferring to a microincubator for dynamic imaging under the OCT microscope. To validate cell migration, laser-scanning confocal microscopy was also used to image the 3-D tissue models. The cells were stained with CellTracker CMTMR (Invitrogen Corp., Carlsbad, CA) before being mixed with gel. Time-lapse confocal image z-stacks were obtained every 3 minutes.

2.3 Cell Proliferation Assay

Tissue models made of 3T3 fibroblasts and Matrigel gel were used in the cell proliferation assay. The tissue models were cultured in an incubator, and periodically removed for OCT imaging. OCT images were used to estimate the cell number increase in 3-D tissues. Similar samples were used for histological analysis. Frozen sections were stained with hematoxylin-eosin (H&E) for white-light histological observations.

2.4 Cell De-Adhesion Assay

The tissue model was made by seeding 5×10^4 3T3 fibroblasts in a 3-D calcium phosphate scaffold (BD Bioscience, Bedford, MA). After culturing for ten days to achieve a high cell density, the tissue was immersed in the solution of 0.25% trypsin/EDTA. The tissue model was immediately and continuously visualized with OCT to track the dynamic process of cell detachment from the scaffold.

2.5 Microstructured Substrate and Mechanical Stimulation

GFP-vinculin transfected fibroblasts cultured on flexible poly-dimethyl-siloxane (PDMS) microtextured substrates with 3-D topographic features were employed to demonstrate the capability of OCT to visualize cell responses to mechanical stimuli. The mechanical stimulation system, a StageFlexer system (Flexercell Inc. NC) was used to stretch the cells on or cells in 3-D Matrigel. Cells cultured under mechanically-stimulating conditions with the StageFlexer system were subject to equibiaxial cyclic stretching for 24 hours.

2.6 Optical Coherence Tomography

OCT imaging was performed on tissue models. Our fiber-based OCT system used a Nd:YVO₄-pumped titanium:sapphire laser as a broad-bandwidth optical source that produced 500 mW of average power and approximately 90 fs pulses with an 80 MHz repetition rate at an 800 nm center wavelength. Laser output was coupled into an ultrahigh-numerical-aperture fiber (UHNA4, Thorlabs, Inc.) to spectrally broaden the light from 20 nm to more than 100 nm, generating the axial resolution of our system at 3 μm [21]. The reference arm of the OCT interferometer consisted of a galvanometer-driven retroreflector delay line that was scanned a distance of 2 mm at a rate of 20 Hz. The sample arm beam was focused into the tissue by a 12.5 mm diameter, 20 mm focal length achromatic lens to a 10 μm diameter spot size (transverse resolution). The 12 mW beam was scanned over the engineered tissue with

galvanometer-controlled mirrors. The envelope of the interference signal was digitized to 12-bit accuracy.

2.7 Three-Dimensional Data Reconstruction

Three-dimensional images were reconstructed with SliceDicer (Pixotec, Renton, WA) or Amira (Image System, Minnetonka, MN).

3. Results and Discussion

3.1 Cell Migration

The Boyden chamber assay using microporous membrane inserts is the most widely accepted assay for cell migration and invasion [20]. In order to facilitate the dynamic imaging of cells, we fabricated a modified Boyden chamber system for a real-time cell migration assay in 3-D matrices and made it adaptable to a microincubator for long-term cell imaging studies (Fig. 1). The microincubator was placed under an OCT microscope during the entire experimental period, providing cells optimal physiological conditions while migrating. The cells migrate towards the chemo-attractant, MCP-1, and migration parameters were measured with this chemotaxis assay. Figure 2 demonstrates the 3-D positional changes of the cells in the tissue model over time. Cell positions at each specific time-point were labeled with a specific color. Cell migration direction and velocity could be readily obtained from these OCT images. The migration speed in our experiment was approximately $0.03 \mu\text{m}/\text{min}$ ($20 \mu\text{m}$ per 30 min), which correlated with that reported in the literature [22,23]. The migration speed was uniform throughout the 2 mm detection depth. By combining the time-lapse 3-D images into composite images (Figs. 2g and 2h), we can track the paths traveled by individual cells and determine the distribution of phenomenological parameters, including cell speed. The cell migration speed decreased after 2 hours, but the cell density in the gel had increased, which may have been a contributing factor.

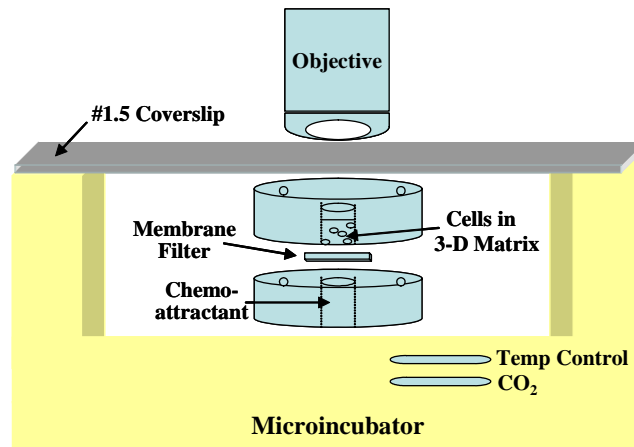


Fig. 1. Experimental set-up for cell chemotactic migration studies. A modified Boyden chamber is shown, in expanded view to show membrane filter, and contained with a microincubator chamber for long-term imaging studies on a microscope stage.

Laser-scanning confocal microscopy was used to image cell migration with a similar setup. However, the imaging configuration of the confocal microscope was inverted, so the entire migration chamber system shown in Fig. 1 was subsequently inverted on the stage, which subsequently resulted in an upward trend in migration (Fig. 3). Compared to the OCT images, confocal images have higher spatiotemporal resolution. The migration speed observed in the confocal imaging studies was similar to that from OCT time-lapse images. Compared to

the OCT imaging technique presented here, current methods of analysis of cell migration and invasion are time-consuming and tedious, involving cotton swabbing of non-migrated cells on the top side of the insert, manual staining, and counting. We present an approach for determining the cell migration speed, direction, and path, and evaluating the effect of isotropic variations in the extracellular environment on the tissue cell motility. OCT imaging provides a wider field-of-view, deeper imaging penetration, and the potential for long-term investigations because no probes or dyes are required. Confocal microscopy, however, in conjunction with dependent expression of fluorescent probes, can provide additional insight into functional parameters.

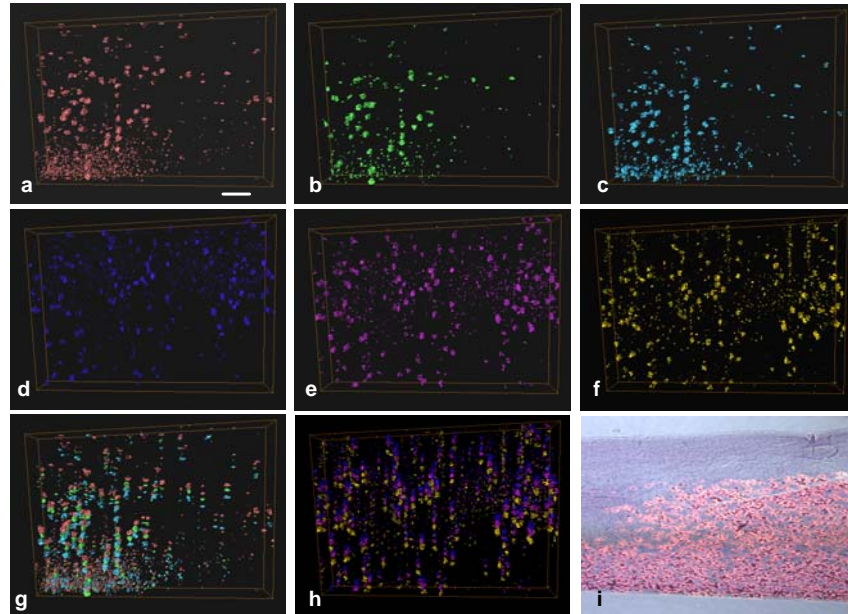


Fig. 2. OCT of cell migration. 3-D OCT images demonstrate the migration of macrophages (a-f). Cells at different points in time are labeled with different colors. The interval time is 40 min between (a/b, b/c, d/e, and e/f), and 120 min between (c/d). Individual OCT images are merged to form composite images of individual cell migration in 3-D space (g,h). Composite (g) is composed of (a-c) and (h) is a composed of (d-f). Corresponding histology after the study is shown in (i), with macrophages collecting at the bottom. Scale bar is 200 μm .

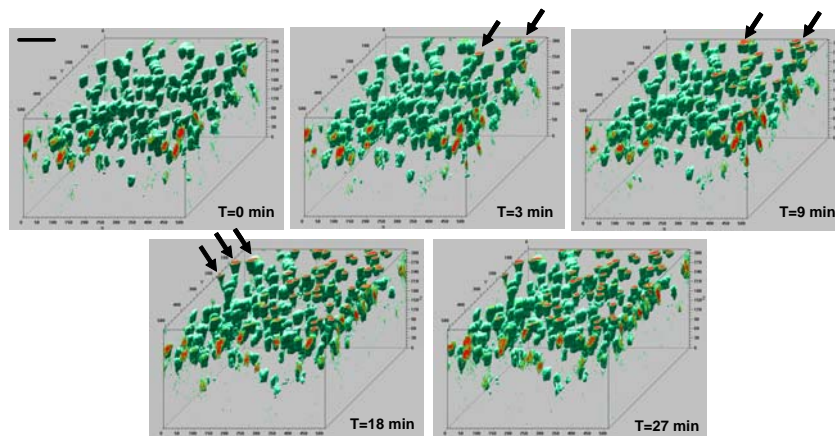


Fig. 3. Cell migration validation with confocal microscopy. 3-D confocal images of cell migration through the matrix is shown. Migration direction is upward as the microincubation chamber was inverted on an inverted microscope stage. Note the increasing number of cells entering the top plane of the volume (arrows) over time. Scale bar represents 50 μm .

Cell migration is an essential function of normal tissue processes, including embryonic development, angiogenesis, and wound healing. For example, the migration of precursor cells from the basal layer to the epidermis functions to continuously renew skin. Cell migration is also a fundamental process that can contribute to important pathologies. Leukocyte migration from the circulation into the surrounding tissue, where they ingest bacteria, is important for mounting an immune response. Chemotaxis assays usually are carried out to study the migration ability of cells in response to a chemical or biological factor. Much of our knowledge regarding migration has been obtained from cells growing on flat surfaces, such as coverslips or tissue culture dishes. Only recently have studies begun to examine migration in environments which more closely mimic that observed *in vivo*, such as 3-D matrices and tissue slice cultures. Migration modes and cell morphologies in 3-D environments can differ significantly from those observed with dissociated cells migrating on planar substrates [24]. Our approach has been through time-lapse 3-D OCT where the migration rates and directionality of cells in 3-D matrices can be readily measured.

This migration assay based on non-invasive optical imaging with OCT provides a quick and efficient system for quantitative determination of factors on cell migration. Furthermore, chemo-attractants are potential therapeutic targets for intervention in wound healing, cancer, and inflammation. Our results suggest that it is possible to use OCT to evaluate the performance of various chemo-attractants.

3.2 Cell Proliferation

Figure 4 illustrates representative OCT images used to track cell proliferation in 3-D tissue models. Both 2-D x-z images and 3-D reconstructed volumes are shown to demonstrate the cell proliferation. Compared to the cells cultured on a monolayer, cells seeded in a 3-D matrix might encounter matrix resistance to migration. Thus, cells divide and form aggregates at the original sites in the matrix. After days of proliferation, the tissue model is comprised of cell aggregates and exhibits a more heterogeneous cell distribution. Therefore, the cell number increase is demonstrated by the increasing size of the cell aggregates in 3-D OCT images.

Due to the limits of the OCT axial and transversal resolution (3 μm and 10 μm , respectively), small gaps among the cells cannot be observed. Thus, single cells in close proximity cannot be resolved. As a result of proliferation, growing clusters or aggregates of cells were seen in the images. Nevertheless, the cell proliferation rate may still be quantified by the diameter of the cell aggregate assuming that the gaps among the cells are much smaller than the cell diameters. Because of the 3-D structure, changes in the scattering volume, instead of the scattering area, should be used in the proliferation measurement. In this case, we estimated the proliferation rate in the tissue model with low initial cell density from Day 0 to Day 3 was 4 times, and that from Day 3 to Day 6 was 4 times as well. The results were confirmed using the histological analysis. This proliferation rate is typical for cells within engineered tissue scaffolds, but is highly dependent on the cell type, microenvironment, and culture conditions.

Cell proliferation provides tissue engineering researchers with the comprehensive level of information on biochemical environments for cell growth. In addition, cell proliferation is an important measurement in cell-based screening for efficiency of therapeutic drugs (e.g. drugs for cancer). Histological assays only provide end-point information. The OCT image approach can provide a real-time, straightforward, and accurate estimation of cell number and proliferation rate in 3-D tissue models.

3.3 Cell De-Adhesion

For cell de-adhesion assays, tissue models were incubated with 0.25% trypsin/EDTA at room temperature. Figure 5 shows the process of cell detaching from the calcium phosphate scaffold. In response to the trypsin-EDTA, it was observed that layers of cells were gradually de-adhered from the 3-D scaffold over the time. The images shown were taken after 10 min, with little change noted in the images before 10 min. OCT imaging of de-adhesion of cells

could be observed based on the optical scattering changes of the tissue in the OCT images. Comparing images at different points of time, the loss of optical scattering, which implies the loss of cells on the scaffold could be assessed (data not shown). For tissue models with high cell density, it is apparent that cells had formed multiple layers on the scaffold. Dynamic OCT imaging of the model demonstrates the dynamic de-adhesion process of the cell layers off of the scaffold.

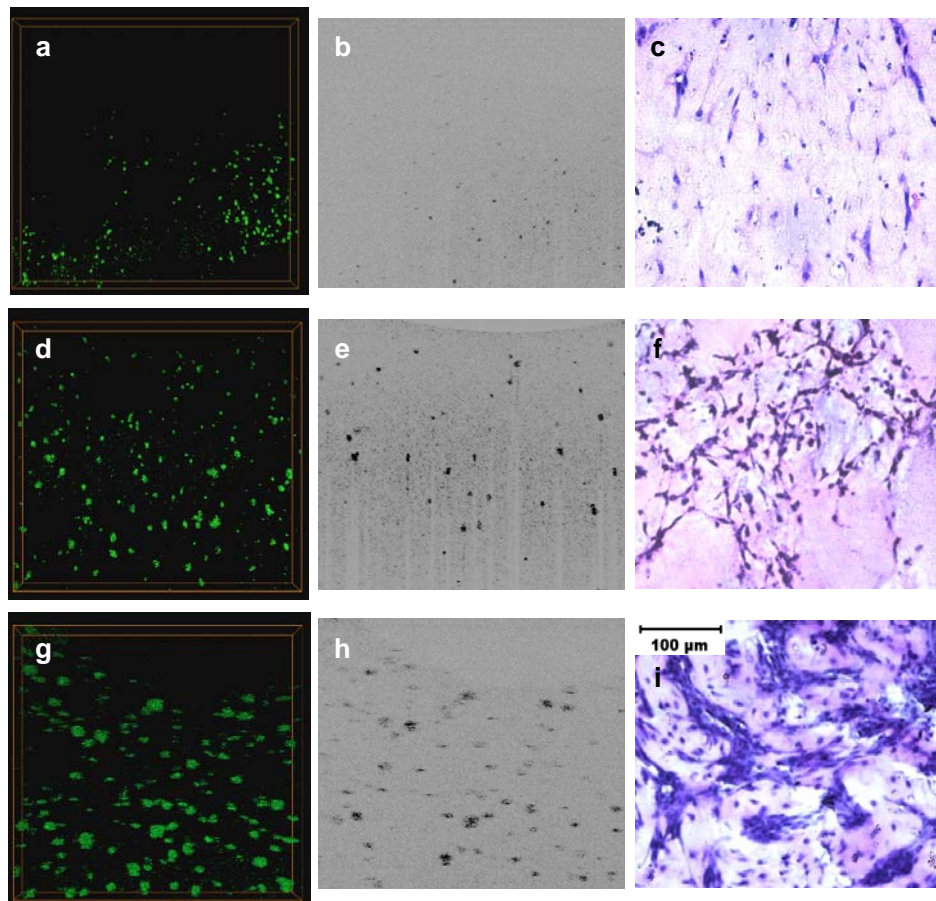


Fig. 4. OCT of cell proliferation in 3-D scaffolds. Images were acquired with low (5×10^4 cells) initial cell density. 3-D OCT images (a,d,g) and 2-D (x-z) OCT images (b,e,h) of engineered tissues were acquired on Day 0 (a-c), Day 4 (d-f), and Day 8 (g-i). Histological images stained with H&E (c,f,i) are shown to confirm cell proliferation over time. Scale bar in (i) is applicable for all images.

Cell adhesion and de-adhesion are fundamental processes that are critically involved in embryonic development and many diseases. One of the most important properties of cells that are derived from multicellular organisms is their ability to adhere to and migrate through extracellular matrices and 3-D structures. OCT has the potential for following these dynamic processes in the developing engineered tissue model, particularly where artificial scaffolds play a central role for defining the early morphology of the tissue.

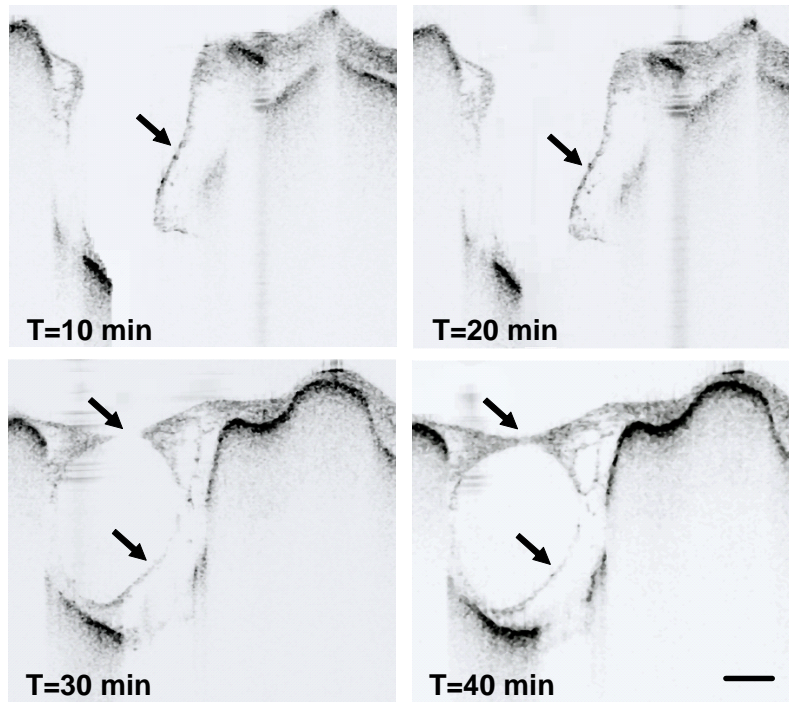


Fig. 5. OCT of cell de-adhesion. Time-lapse images showing the process of cell de-adhesion and cell layer movement (arrows) from a calcium-phosphate scaffold. Continuous images were taken every minute after engineered tissues were soaked in a trypsin solution. Scale bar represents 200 μm .

3.4 Cell-Material Interaction

Cells seeded on microtextured substrates were used to examine the cell-material (structure) interactions (Figure 6). The substrates were characterized by an array of parallel microgrooves with dimensions of $15\ \mu\text{m} \times 15\ \mu\text{m} \times 15\ \mu\text{m}$ (width x height x spacing). Compared to phase-contrast microscopy, OCT can reveal the interactions between the cells and the microstructure in topographic substrates (Fig. 6d) and in 3-D (Figs. 6e, g). OCT images can also demonstrate the changes of cell-material interactions after cultures were stretched for 24 hours. Before being stretched, the cells have a visualized adhesion on the microgrooved structures (Figs. 6c, h). In the OCT image, the cells spread and extended to the bottom of the microstructure (as shown with arrows in the figure), and thus represent active interactions with the structure. This result can be confirmed using fluorescence microscopy that images the GFP-labeled vinculin (cell focal adhesion sites) in these transfected cells (Fig 6j). However, equibiaxial strains cause the cells to dissociate from the structure and form clusters (Fig 6i, k). A possible reason is that the microgrooves direct the cells to one direction while physically limiting the extension in the other directions. Equibiaxial strains may force the cells to rearrange their orientation according to the strain field, which caused the cells to grow on top of the groove structure instead of interact with the 3-D structure.

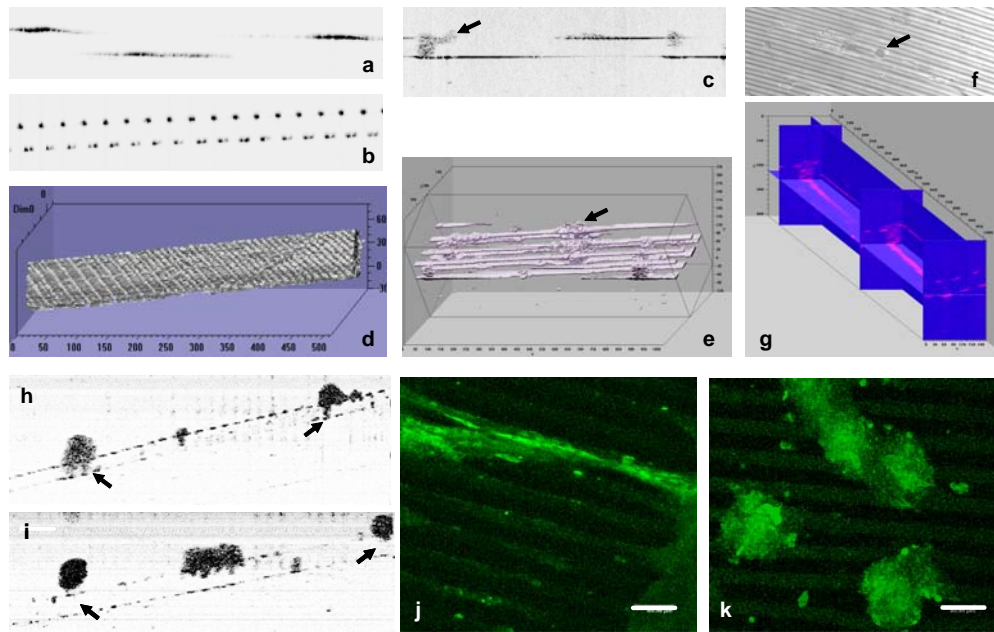


Fig. 6 OCT imaging of cell-substrate interactions. 2-D (a-c) and 3-D (d) OCT images of microtextured (microgrooved) PDMS substrates used for cell culture (e,g,h,i). OCT images (a-e, g-i) were compared with corresponding phase contrast (f) and fluorescence microscopy (j,k) images. Individual cells are indicated by arrows. Mechanical effects on cell-substrate interactions are visualized (h-k). Images are also shown before (h,j) and after (i,k) 5% equibiaxial stretching. Scale bar represents 80 μm .

3.5 Matrix Influencing Effects

During these investigations, we found that the matrix composition significantly influences the signal content within OCT images (Fig. 7), which is relevant to other investigators wishing to pursue cell-imaging studies with OCT. The addition of collagen I reduces the visibility of cells in the 3-D matrix. This may be caused by the scattering effects specific to the collagen, which may have similar optical scattering properties as the cells. This suggests a potential limitation of OCT systems for the real-time imaging of cell activities in 3-D tissue models over time. Matrix materials must be selected to have different scattering properties from the cells and from the extracellular matrix that is gradually secreted by proliferating cells over time.

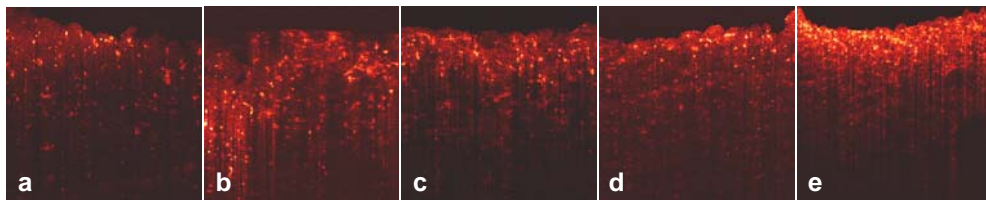


Fig. 7. Collagen-dependent changes in OCT. OCT images of tissue models are shown with a constant cell number ($\sim 5 \times 10^4$) and increasing amounts of collagen in the Matrigel matrix. Collagen percentage varies for (a) 0%, (b) 0.05%, (c) 0.1%, (d) 0.15%, and (e) 0.2%. Increasing collagen content increases scattering, reducing imaging depth and contrast between cells and matrix.

4. Conclusion

Visualizing the 3-D organization and dynamics of cells in relation to their surrounding biochemical and biomechanical environments in an unperturbed or perturbed context requires a noninvasive, high-resolution, imaging technique. In this paper, we described our approach which uses a four-dimensional (3-D space over time) high-resolution OCT system in conjunction with 3-D cell and tissue culture and assay techniques. We demonstrate that OCT, frequently used for generating histology-like images of tissue structure, can be used to track and analyze cell dynamics in tissue models.

Three-dimensional cell-based tissue models have become increasingly useful in the fields of tissue engineering, drug discovery, and cell biology. While techniques for building these tissue models have advanced, there has been an increasing demand for imaging techniques that are capable of assessing complex 3-D cell behaviors in real-time, and at the depths that comprise thick tissues. Understanding these cell behaviors requires advanced imaging tools to progress from characterizing 2-D cell cultures to more complex, highly-scattering, thick 3-D tissue constructs. OCT is an emerging biomedical imaging technique that can perform cellular-resolution imaging in living and developing tissue models in real-time. We have demonstrated that it is possible to use OCT to evaluate dynamic cell behavior and function in a quantitative fashion in four dimensions (3-D space over time). This powerful approach to the noninvasive imaging of the morphology and function of tissue models has enormous potential for a wide range of applications ranging from tissue engineering to drug discovery.

Acknowledgments

We wish to thank Dr. Daniel Marks of the Beckman Institute for Advanced Science and Technology for his technical contributions to the image acquisition software and for his intellectual contributions to the design of this imaging system. This work was supported in part by the National Institutes Health (NIBIB, 1 R01 EB00108, S.A.B.), and the University of Illinois Critical Research Initiative (S.A.B.). Dr. Wei Tan is currently at the University of Colorado at Boulder, Department of Mechanical Engineering. Additional information can be found at <http://biophotonics.uiuc.edu>.